

ISSI

Manifold Iodine Cell

Operating Instructions (Version 1.0)



Table of Contents

Description	2
Specifications.....	2
Background	3
Procedure to Set Manifold Iodine Cell	4
Dimensions	5
Export Disclaimer.....	6

For questions or comments, please contact ISSI

Innovative Scientific Solutions, Incorporated

7610 McEwen Road

Dayton, OH 45459

Ph.: (937) 630-3012

Fax: (937) 630-3015

Email: issi-sales@innssi.com

www.innssi.com

Revision Date: 9/25/2017

Description

Iodine-vapor cells with a manifold are 3-in.-dia, 5-in.-long or 10-in.-long Pyrex cells. Standard cells are manufactured with 1/4 gm of iodine (actual pressure determined by temperature of water cooling jacket at the time of operation). In addition, transitions can be pressure broadened with buffer gas supplied by user through a fill-port.




Specifications

Length	125-mm or 250-mm
Diameter	76-mm
Housing	Anodized Aluminum
Mounting	¼"-20
Maximum Operating Temperature	130 °C
Set Point	30°C - 50°C
Thermocouple	Type T
Temperature Controller	Optional add-on
Input Power	110 VAC, 60 Hz
Warranty	1 year
ECCN	EAR99

Background


To create a sealed starved cell with a flexible set point, a glass cell with an attached cold-finger and vacuum port is constructed. The vacuum port and cold-finger include stopcocks. The cell is evacuated and cold-finger filled with iodine is brought to the desired vapor pressure (cold-finger operating temperature). The stem between the cold-finger and cell is then closed by closing the stopcock, isolating the iodine in the cell body and fixing the number density. The cell is then operated 10-20 °C above the cold-finger set temperature and the iodine in the cell is a super-heated vapor with a set number density. The result is a molecular cell with a very stable absorption spectra.

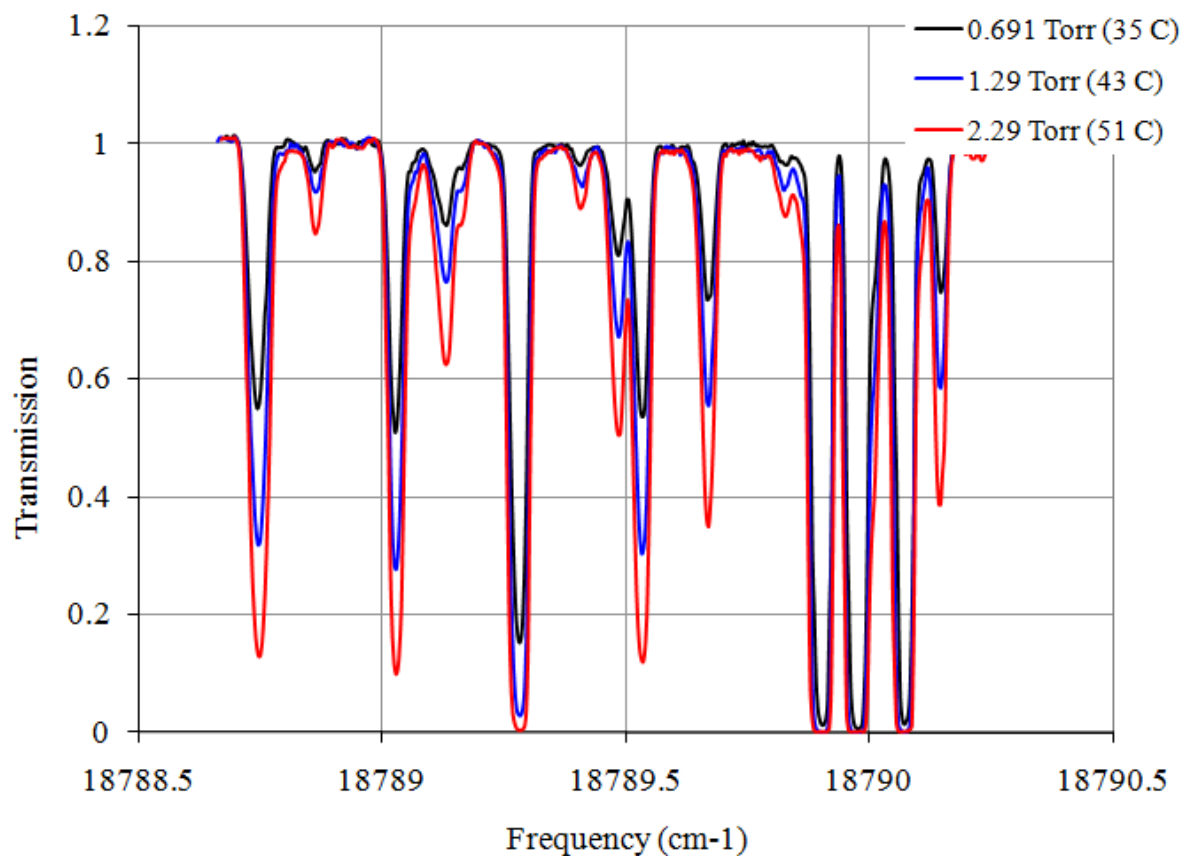


Procedure to Set Manifold Iodine Cell

- 1.) Close both stopcocks
 - Never open the vacuum and iodine stopcocks at the same time or you will drain the iodine from the cell
- 2.) Connect the temperature controlled water bath to the water bath connectors
 - This is used to set the iodine pressure/density
- 3.) Turn on the water bath
- 4.) Connect the vacuum pump connector to a vacuum pump
 - If using an oil based pump, make sure it has a sieve or trap to prevent oil from contaminating the cell
- 5.) Turn on the vacuum pump
- 6.) Turn on the cell heater, set temperature to at least 25 C above the water bath set point
 - A low cell temperature will result in iodine condensing on the cell windows
- 7.) Allow the cell body temperature, water bath temperature to reach steady state
 - give the system about 30 min
- 8.) Open the vacuum stopcock
 - Allow the pump to pull on the cell for 10-15 min with the cell heated
- 9.) Open the iodine stopcock and then close the vacuum stopcock
 - Allow the iodine to reach equilibrium (about 3-5 min)
- 10.) Close the iodine stopcock
- 11.) With both stopcock closed, system can be shut down and disconnected

Dimensions

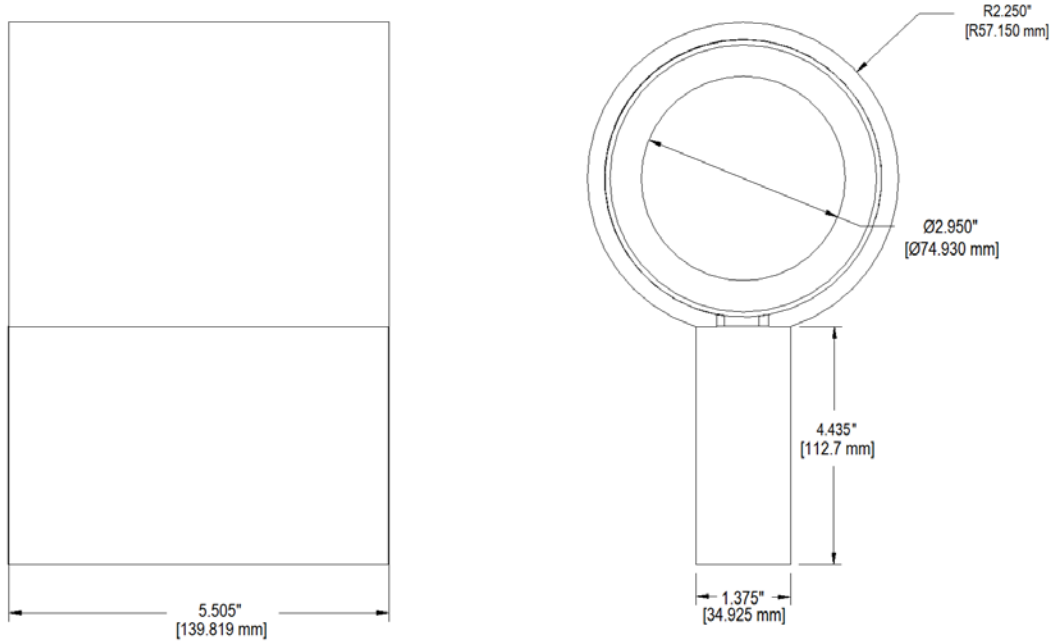

5-inch, Manifold Iodine Cell (I2M-5)

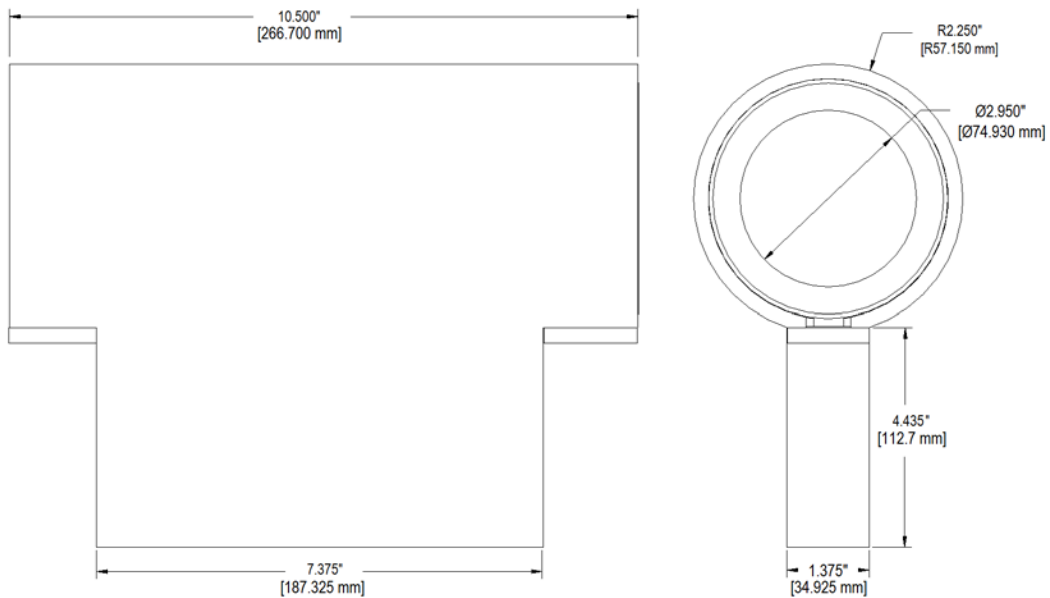

10-inch, Manifold Iodine Cell (I2M-10)

Export Disclaimer

Any and all underlying information and technology contained in this document may be subject to U.S. export controls, including the Export Administration Act (50 U.S.C. Appx. §§ 2401 et seq.) and the Export Administration Regulations ("EAR", 50 C.F.R. Parts 730-774), and may be subject to export or import regulations in other countries. You are responsible for complying with all trade regulations and laws both foreign and domestic. Except as authorized by law or distributor agreement with ISSI, you agree and warrant not to export or re-export the information to any country, or to any person, entity, or end-user subject to U.S. export controls, including without limitation persons or entities listed on the U.S. Department of Commerce Bureau of Export Administration's Denied Parties List and the U.S. Department of Treasury's Specially Designated Nationals. You further represent and warrant that no U.S. federal agency has suspended, revoked, or denied your export privileges.